



## 人的趋化蛋白 12 定量分析酶联免疫检测试剂盒

本试剂盒仅供科研使用。用于体外定量检测人血清、血浆或细胞培养上清液中的 CXCL12 浓度。**使用前请仔细阅读说明书并检查试剂组分是否完整。**如有产品包装破损或质量投诉，请在收到货一个月之内联系我们。

### CXCL12 简介:

CXCL12, 也叫 SDF-1, 属于 CXC 趋化因子家庭。由位于 10 号染色体的 CXCL12 基因编码。有两种亚型 SDF-1 $\alpha$  和 SDF-1 $\beta$ , SDF-1 $\alpha$  是一个 89 个氨基酸的多肽, SDF-1 $\beta$  与 SDF-1 $\alpha$  相比, 序列相同, 只在 C 末端多了 4 个残基。SDF-1 $\alpha$  是一个高度保守的蛋白, 在人和小鼠间有 99% 的同源性。

SDF-1 由骨髓基质细胞表达, 在包括心、肝、脑、肾、骨骼肌和淋巴器官等许多器官都存在。

SDF-1 作为一个高效的淋巴细胞趋化因子, 能直接诱导和活化淋巴细胞在 LPS、TNF 和细胞因子等的免疫刺激作出应答, SDF-1 作为单核细胞有效的化学诱导剂, 能刺激 B 细胞增殖。SDF-1 似乎在淋巴细胞和造血细胞的运输和归巢中有一定的作用。SDF-1 已证明在肿瘤发生的过程中有重要的作用, 包括刺激肿瘤细胞的生长、恶化、促进肿瘤血管增生、肿瘤转移等生理过程均有刺激作用。

### 检测原理:

本试剂盒采用双抗体夹心 ELISA 法检测样本中 CXCL12 的浓度。CXCL12 捕获抗体已预包被于酶标板上, 当加入标本或参考品时, 其中的 CXCL12 会与捕获抗体结合, 其它游离的成分通过洗涤的过程被除去。当加入生物素化的抗人 CXCL12 抗体后, 抗人 CXCL12 抗体与 CXCL12 结合, 形成夹心的免疫复合物, 其它游离的成分通过洗涤的过程被除去。随后加入辣根过氧化物酶标记的亲合素。生物素与亲合素特异性结合, 亲合素连接的酶就会与夹心的免疫复合物连接起来; 其它游离的成分通过洗涤的过程被除去。最后加入显色剂, 若样本中存在 CXCL12 将会形成免疫复合物, 辣根过氧化物酶会催化无色的显色剂氧化成蓝色物质, 在加入终止液后呈黄色。通过酶标仪检测, 读其 450nm 处的 OD 值, CXCL12 浓度与 OD<sub>450</sub> 值之间呈正比, 通过参考品绘制标准曲线, 对照未知样本中 OD 值, 即可算出标本中 CXCL12 浓度。

### CXCL12 定量分析酶联免疫检测试剂盒组成:

组分	规格 (96T/48T)
人 CXCL12 预包被板	12 条/6 条
样本分析缓冲液	5ml/3ml
5 $\times$ 标准品稀释液	10ml/5ml
人 CXCL12 标准品	2 支/1 支 (冻干)
人 CXCL12 生物素化抗体	10ml/5ml
亲和素连接的 HRP 酶	10ml/5ml
浓缩洗涤液 20 $\times$	30ml/15ml
TMB 底物	10ml/5 ml
中止液	5ml/3 ml
封板胶纸	3/2 张
说明书	1 份

### 标本收集:

- 标本的收集请按下列流程进行操作:
  - 细胞上清标本离心去除悬浮物后即可;
  - 血清标本应是自然凝固后, 取上清, 避免在冰箱中凝固血液;
  - 血浆标本, 推荐用 EDTA 的方法收集;
  - 若待测样本不能及时检测, 标本收集后请分装, 冻存于 -20 $^{\circ}$ C, 避免反复冻融。
- 血清标本不应添加任何防腐剂或抗凝剂;
- 标本应清澈透明, 检测前样本中如有悬浮物应通过离心去除。



4. 请勿使用溶血，高血脂或污染的标本检测，否则结果将不准确。


**注：人血清或血浆样本请用样本分析缓冲液做倍比稀释后再检测。**

### 注意事项：

1. 试剂盒请保存在2~8℃。
2. 浓缩洗涤液因在低温下可能有结晶，请水浴加热使结晶完全溶解后再配制工作液。
3. 标准品复溶加样后，剩余部份请丢弃。
4. 底物请勿接触氧化剂和金属。
5. 加样时，请及时更换枪头，避免交叉污染。
6. 严禁混用不同批号的试剂盒组份。
7. 充分混匀对保证反应结果的准确性很重要，在加液后请轻轻叩击边缘以保证混匀。
8. 室温反应，请严格控制在25~28℃。
9. 洗涤过程是至关重要的，洗涤不充分会使精确度下降并导致结果误差较大。
10. 试验中标准品和样本检测时建议作双复孔。
11. 加样过程中避免气泡的产生。
12. 血清和血浆标本的检测时，检测抗体的孵育时间应适当延长。

### 检测前准备工作：

1. 试剂盒自冰箱中取出后应置室温（25~28℃）平衡20分钟；每次检测后剩余试剂请及时于2~8℃保存。
2. 将浓缩洗涤液用双蒸水或去离子水稀释（1份加19份水）。
3. 将5×标准品稀释液用双蒸水或去离子水稀释（1份加4份水）。
4. 标准品：按标签复溶体积加入1X标准品稀释液复溶使CXCL12终浓度达到2000pg/ml，室温反应，请严格控制在25~28℃，静置15~20分钟后轻轻混悬（建议抽取几次）待彻底溶解，用标准品稀释液倍比梯度稀释后依次加入检测孔中。（标准曲线取七个点，最高浓度为2000 pg/ml，标准品稀释液直接加入作为0浓度。）

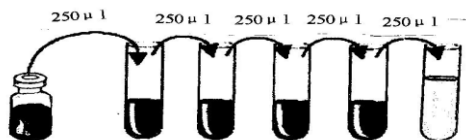

### 洗涤方法：

自动洗板机或人工洗板：每孔洗涤液为300u1，注入与吸出间隔15-30秒。洗板5次。最后一次洗板完成后将板倒扣着在厚吸水纸上用力拍干。

### 实验过程需自备的材料：

1. 不同规格的加样枪及相应的枪头；
2. 酶标仪；
3. 自动洗板机；
4. 去离子水或双蒸水；

### 操作步骤：

1. 通过计算并确定一次性实验所需的板条数，取出所需板条放置在框架内，暂时用不到板条请放回铝箔袋密封，保存于4℃。
2. 建议设置本底校正孔，即空白孔，设置方法为该孔只加TMB显色液和中止液。每次实验均需做标准品对照并画出标准曲线。
3. 分别将标本或不同浓度标准品（100u1/孔）加入相应孔中，用封板胶纸封住反应孔，室温（25~28℃）孵育120分钟。如果是血清血浆样本，不同样本稀释比例不一样，一般范围在5~20倍，如无明确范围，建议从2倍开始，加样稀释说明如下：每孔先加样本分析缓冲液50u1，再加用1×标准品稀释液稀释1倍后的样本，加样量为50u1。
4. 洗板5次，且最后一次置厚吸水纸上拍干。
5. 加入生物素化抗体工作液（100u1/孔）。用封板胶纸封住反应孔，室温（25~28℃）孵育60分钟。
6. 洗板5次，且最后一次置厚吸水纸上拍干。
7. 加入亲和素连接的HRP酶工作液（100u1/孔）。用封板胶纸封住反应孔，避光室温（25~28℃）孵育20分钟。



8. 洗板5次，且最后一次置厚吸水纸上拍干。
9. 加入显色剂TMB100u1/孔，避光室温（25-28℃）孵育20分钟。
10. 加入中止液50u1/孔，混匀后即刻测量OD450值。


### 结果判断：

1. 复孔的值在20%的差异范围内结果才有效，复孔的值平均后可作为测量值。
2. 每个标准品或标本的OD值应减去本底校正孔的OD值。
3. 手工绘制标准曲线。以标准品浓度作横坐标，OD值作纵坐标，以平滑线连接各标准品的坐标点。通过标本的OD值可在标准曲线上查出其浓度。
4. 若标本OD值高于标准曲线上限，应当稀释后重测，计算浓度时应乘以稀释倍数。

#### 典型数值和参考曲线

浓度pg/ml	典型OD值1	典型OD值2	OD平均值
0	0.1126	0.1293	0.12095
62.5	0.2139	0.2534	0.23365
125	0.3398	0.3864	0.3631
250	0.5283	0.5749	0.5516
500	0.8587	0.9672	0.91295
1000	1.3321	1.419	1.37555
2000	1.9364	1.9814	1.9589

#### 人CXCL12参考标准曲线

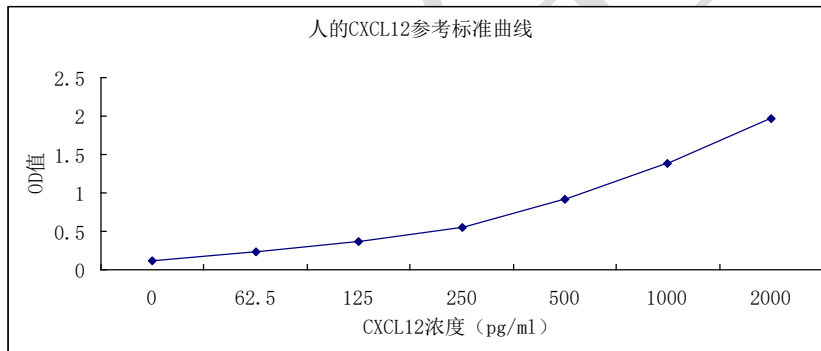

**注意：**本图仅供参考，应以同次试验标准品所绘标准曲线计算标本含量

#### 灵敏度，特异性和重复性：

1. 灵敏度：多次重复结果表明，最小检出量为22.7pg/ml。
2. 特异性：与人和鼠的IP-10/CRG-2均无交叉反应性，能识别小鼠的SDF-1 $\alpha$ 。
3. 重复性：板内，板间变异系数均<10%。

#### 参考文献：

1. Abi-Younes, S. (2000) Circ. Res. 86(2):131.
2. Sapede, D. et al., 2005, Proc. Natl. Acad. Sci. USA. 102: 1714-1718.
3. Delgado, M.B. et al., 2001, Eur. J. Immunol. 31: 699-707.
4. Bluel, C. et al. (1996) J. Exp. Med. 184:1101.
5. Crump, M.P. et al. (1997) EMBO J. 16:6996.
6. Bbalabian, K. et al., 2005, J. Biol. Chem. 280: 35760-35766.
7. Vila-Coro, A.J. et al. (1999) FASEB J. 13:1699.
8. Oberlin, E. et al. (1996) Nature 382:833.
9. Orimo, A. et al., 2005, Cell. 121: 335-348.
10. Kryczek, I. et al., 2007, Am. J. Physiol. Cell. Physiol. 292: C987-995.



## ELISA Kit for the Quantitative Analysis of Human CXCL12

The human CXCL12 ELISA (enzyme-linked immunosorbent assay) kit is used for detection of human CXCL12 in cell culture supernatants, human serum and plasma. THE ELISA KIT IS FOR RESEARCH USE ONLY. Please read this instruction

manual carefully and check out the material provided before use, and you can contact with our company if any questions. You can enter our website or call us for other aim.

### Introduction

CXCL12 also known as SDF-1 is belonging to the CXC chemokine family. It is encoded by the CXCL12 gene which is on chromosome 10. There are two alternatively spliced variants of SDF-1 (1), SDF-1 $\alpha$  and SDF-1 $\beta$ . SDF-1 $\alpha$  is an 89 amino acid polypeptide, while SDF-1 $\beta$  has the identical sequence with a 4-residue C-terminal extension. SDF-1 has a higher degree of inter-species conservation with 99% identity between the human and the mouse sequences (1, 3).

SDF-1 is constitutively expressed by bone marrow stromal cells and is present in various organs including heart, liver, brain, kidney, skeletal muscle, and lymphoid organ.

As a highly efficacious lymphocyte chemoattractant, CXCL12 / SDF-1 activates and directs the migration of leukocytes in response to proinflammatory stimuli such as LPS, TNF, or interleukins. It is a potent chemoattractant for monocytes, and it enhances B-cell proliferation (1, 2, 4), SDF-1 appears to play a role in trafficking or homing of lymphocytes and hematopoietic cells (8). SDF-1 has been demonstrated that CXCL12 / SDF-1 promotes tumor growth and

malignancy, enhances tumor angiogenesis, participates in tumor metastasis, and thus plays an important role in carcinoma pathogenesis.

### Principles of the Test

The kits is a solid sandwich enzyme-linked immunosorbent assay for detection of human CXCL12. An anti-human CXCL12 monoclonal antibody has been absorbed onto the wells of the microtiter strips provided. Samples including specimens or standards were pipetted into wells. The human CXCL12 in specimens or standards would be captured by the coated antibody and the free others were removed by washing. The human CXCL12 biotin-conjugated antibody were added and binds to human CXCL12 captured by the first antibody, which formed a sandwich. Streptavidin-HRP would be added and binds to the biotin conjugated antibody, then free Streptavidin-HRP would be removed during a wash step. After this, substrate solution would be added and catalyzed by the HRP, and a coloured product is formed. The intensity of the colored product is used to calculate in proportion to the amount of human CXCL12 in the original specimen.

### Materials provided with the kits

Reagent	96/48 Test Kit
Assay Buffer	5ml/3 ml
Human CXCL12 Antibody-Coated Wells	12 strips/6 strips
Standard Diluent	10 ml/5ml
Human CXCL12 Standard	2/1 vial(s)
Human CXCL12 Detection Antibody	10ml/5ml
Streptavidin-HRP	10ml/5ml
Wash Buffer Concentrate 20x	30ml/15ml
TMB	10ml/5 ml
Stop Solution	5ml/3 ml
Plate Covers	3/2
Complete Instruction Manual	1



## Specimen Collection

1. Collecting specimen as following:

- A. The particulate of the cell culture supernatants should be removed before use.
- B. Serum was obtained from clot at room temperature.
- C. Please collect plasma with EDTA.
- D. Assay immediately or store samples at  $-20^{\circ}\text{C}$ . Avoid free-thaw cycles.

2. Antiseptic and anticoagulant should not appear in Serum samples.
3. Any particulate should be removed from samples before use.
4. Do not use grossly hemolyzed or lipemic samples.

**Note: Strongly recommend that the serum and plasma samples should be diluted as doubling dilution before use.**

## Precautions for use:

1. Please storage the Kit at  $2\sim 8^{\circ}\text{C}$ .
2. Washing buffer concentrate may have crystal in low temperature, and you can melt its in water-bath before use.
3. Please discard the remains after use of the dissolved standard.
4. Avoid contact of substrate solution with oxidizing agents and metal.
5. Usage of disposable pipette tips avoid microbial contamination or cross-contamination of reagents or specimens.
6. Do not mix or substitute reagents with those from other lots or other sources.
7. To ensure the adequate mixture of added reagents, please tap gently the plate after the wells were filled with liquid.
8. Incubation temperature should be  $25\sim 28^{\circ}\text{C}$ .
9. Wash step was crucial for whole assay process.
10. Duplicate wells of the same sample were recommended in assay process
11. Avoid the foam while pour the liquid into wells.
12. For serum or plasma samples, the biotin-conjugated antibody should be incubate for at least 90 minutes.

## Reagent Preparation

1. The reagents should be warmed up to room temperature before use. The remanent reagents must reseal and put into refrigeratory again as soon as possible.
2. Dilute 1ml of wash buffer Concentrate into 19ml deionized or distilled water to work.
3. Dilute 1ml of  $5\times$  sample diluent into 4ml deionized or distilled water to  $1\times$  sample diluent.
4. Add sample diluent to the bottle according to the volume of the label and wait 15 minutes for complete dissolution. Incubation temperature should be  $25\sim 28^{\circ}\text{C}$ . And in turn add the half concentration diluent by standard diluent.

## Wash step:

Automated microplate washer or operating by pipette: Each well should be pour into 300ul wash buffer and soak 15 or 30 seconds, then be aspirated, five times process were repeated. After the last wash, remove remaining wash buffer by aspirating. Invert the plate and blot it against clean paper towels.

## Materials Required But Not Provided

1. pipettes and pipette tips
2. Microwell strip reader capable of reading at 450 nm (540 nm as optional reference wave length)
3. automated microplate washer
4. Glass-distilled or deionized water

## Assay procedure

1. The needed strips were putted into the frame, the remains were returned into foil pouch and resealed.
2. Blank well were recommended, which only color reagent and stop solution be added. It is suggested that each testing with gradient density of standard for standard curve.
3. Add 100ul of standard or sample. Cover with the Plate Covers provided. Incubate for 2 hours at room temperature. If the serum levels of plasma samples, different sample dilution ratio is different, generally range in 1~10 times, if there is no definite scope, advice from 2 times, add sample dilution shows as follows: Each hole add buffer 50 ul sample analysis, add in 1 x standard sample after 1 times diluent dilution, and sample amount to 50 ul.
4. Five times wash process were repeated.



5. Add 100ul of detection antibody. Cover with the Plate Covers provided. Incubate for 1 hour at room temperature.
6. Five times wash process were repeated.
7. Add 100ul of Streptavidin-HRP. Cover with the Plate Covers provided. Lucifugal incubation for 20 minutes at room temperature.
8. Five times wash process were repeated.
9. Add 100ul of TMB, Lucifugal incubation for 20 minutes at room temperature.
10. Add 50ul of stop solution to each well, determine the optical density of each well within 10 minutes.


## Calculation of Results

1. Duplicates should be within 20 percent of the mean. Average absorbance values for each set of duplicate samples were used as detection results.
2. The blank absorbance values of subtract should be deducted.
3. Drawing a best fit curve through the points of graph. Draw the standard curve by plotting assayed OD value (on the Y axis) vs. concentration (on the X axis). The sample concentration was obtained based on its OD value founding in the standard concentration curve.
4. If the values obtained are not within the expected range of the standard, Samples should be dilute and assay again.

## Typical Data and Standard Curve

concentration (pg/ml)	Typical data 1	Typical data 2	Average
0	0.1126	0.1293	0.12095
62.5	0.2139	0.2534	0.23365
125	0.3398	0.3864	0.3631
250	0.5283	0.5749	0.5516
500	0.8587	0.9672	0.91295
1000	1.3321	1.419	1.37555
2000	1.9364	1.9814	1.9589

## Human CXCL12 Standard Curve

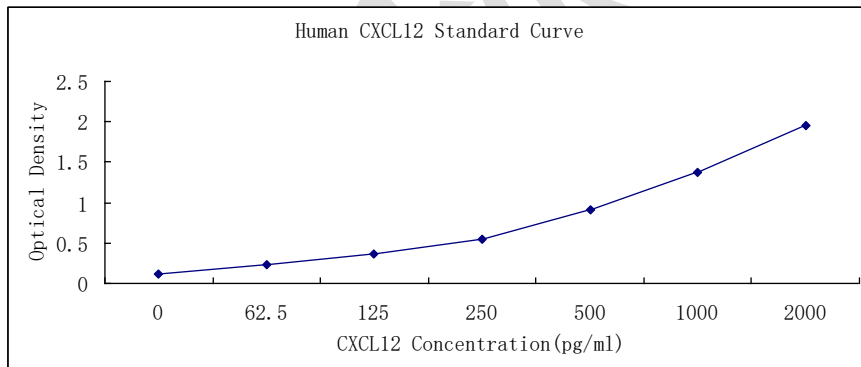

## Sensitivity, Specificity, Repeatability

**Sensitivity:** repeated assays were evaluated and the minimum detectable dose was 22.7pg/ml.

**Specificity :** No significant cross-reactivity or interference with human and mouse IP-10/CRG-2. Can identify the mouse SDF - 1 alpha

**Repeatability:** The coefficient of variation between wells or plates is less than 10 percent.

## REFERENCES:

1. Abi-Younes, S. (2000) Circ. Res. 86(2):131.
2. Sapede, D. et al., 2005, Proc. Natl. Acad. Sci. USA. 102: 1714-1718.
3. Delgado, M.B. et al., 2001, Eur. J. Immunol. 31: 699-707.
4. Bluel, C. et al. (1996) J. Exp. Med. 184:1101.
5. Crump, M.P. et al. (1997) EMBO J. 16:6996.
6. Bbalabian, K. et al., 2005, J. Biol. Chem. 280: 35760-35766.



上海传秋生物科技有限公司

English name

- 
7. Vila-Coro, A.J. et al. (1999) FASEB J. 13:1699.
  8. Oberlin, E. et al. (1996) Nature 382:833.
  9. Orimo, A. et al., 2005, Cell. 121: 335-348.
  10. Kryczek, I. et al., 2007, Am. J. Physiol. Cell. Physiol. 292: C987-995

上海传秋生物